


-15kV TOF: -9245 v
 -3.6kV MCP: -2593 v
 -2.4kV MCP: -1579 v
 Input Cur: 300 ma
 RPA max: 237 v
 Mirror max: 237 v

Mon Sep 25 10:46:43 2006

TIDE Direct Events

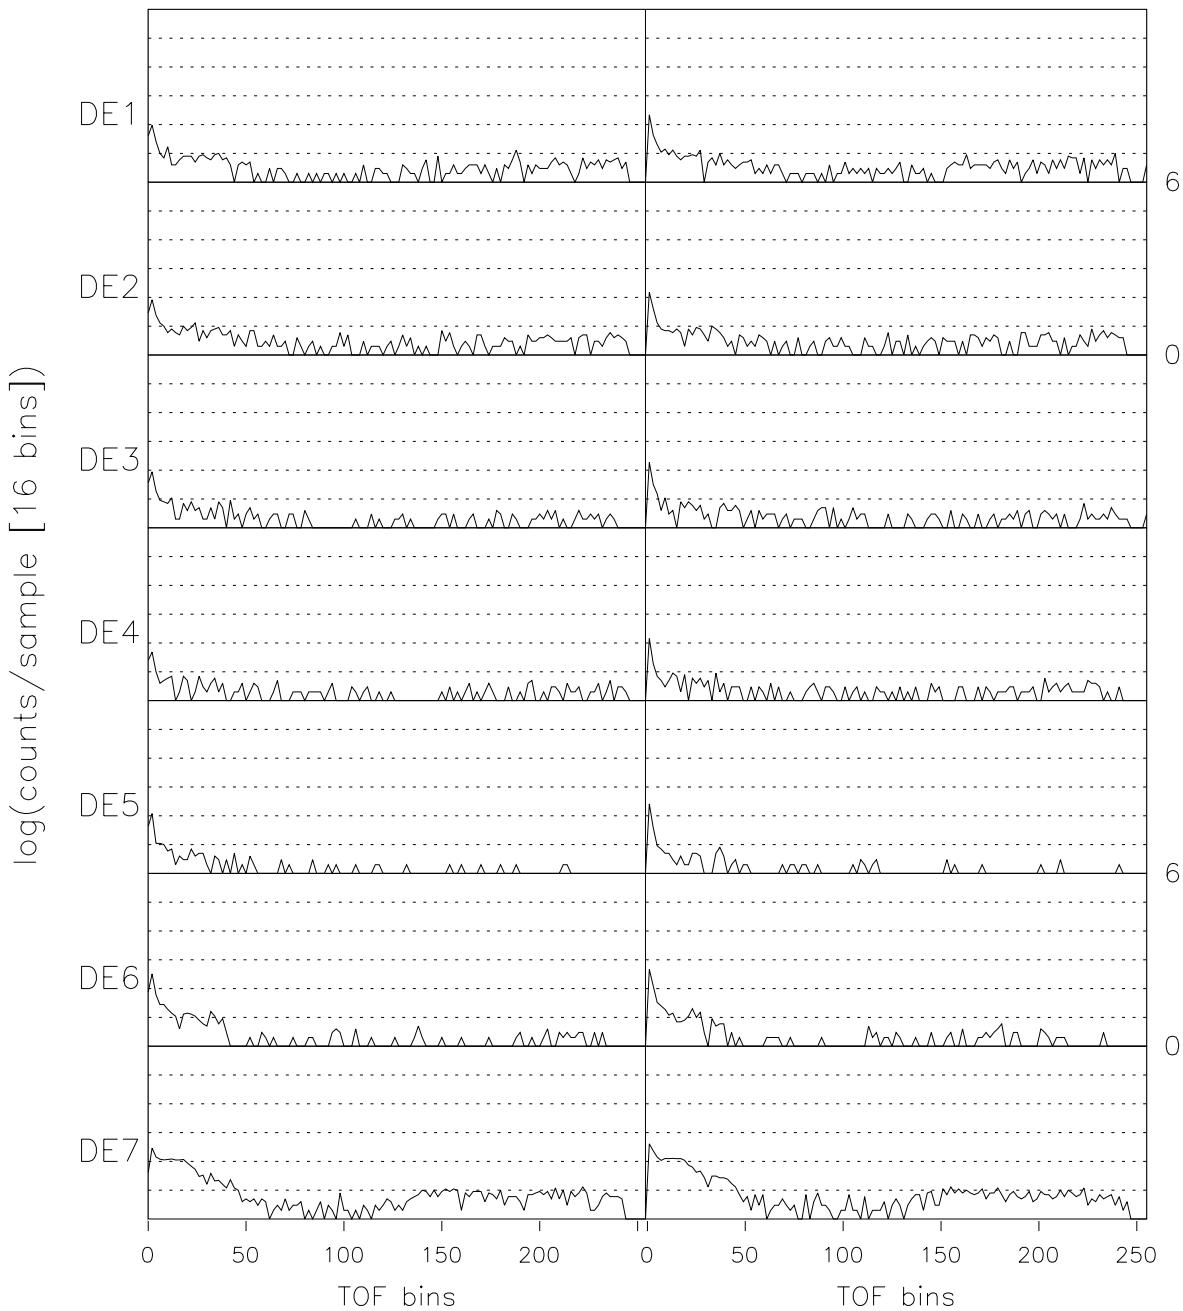

reported: 09-03-96 15:19:00 UT

reported: 09-03-96 15:22:12 UT

file: /export/data/tide/nrt/96090301.dat

-15kV TOF: -9245 v

-3.6kV MCP: -2578 v

-2.4kV MCP: -1579 v

Input Cur: 300 ma

RPA max: 237 v

Mirror max: 238 v